

Operation Manual

Clinical refractometer

It's designed for clinical usage and intended for both Veterinary and Human Being. This unit provides veterinarians and Human Being with quick and accurate indication of vital fluids' levels. Its triple scale reads Urine Specific Gravity(SG), Total Serum Protein(SP) and Refractive Index(RI).



Model	Range	Min. Div.	Accuracy
RHC-200/ATC	0-12g/dl	0.2g/dl	±0.2g/dl
	1.330-1.360RI	0.0005 RI	±0.0005 RI
	1.000-1.050sg	0.005sg	±0.005sg
RDC-300ATC	2-14g/dl	0.2g/dl	±0.2g/dl
	1.000-1.060RI Dog	0.001 RI	±0.001 RI
	1.000-1.060RI Cat	0.001 RI	±0.001 RI

RDC-300ATC: Take care of pets and know their health easily from their vital fluids!


Remarks: 1) If new style model, "N" will be added in the model name, such as RHCN-200ATC etc.. If the model with LED, it is the ZGR models, such as ZGRC-200 ATC etc.

2) ATC Compensation Range: From 10°C to 30°C (50°F to 86°F)

Parts:

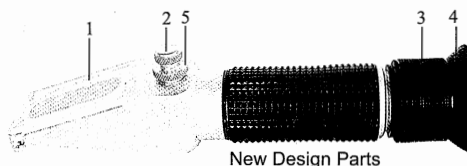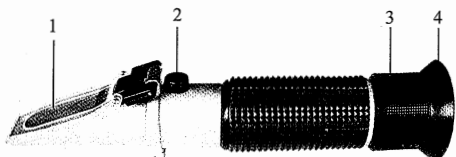

- 1----Daylight Plate;
- 2----Calibration Screw;
- 3----Focus Adjustment;
- 4----Eyepiece;
- 5----Calibration screw lock
- 6----Power Switch(+);
- 7----Battery cell cover
- 8----LED light

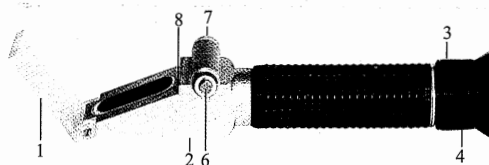


Remarks for ZGR series only

- Power Require: 3 "AAA" Button Cell (1.5V*3)
- Battery Life: More than 100hours
- Light Source: White LED



RHCN-200ATC Catalogue No: 1841

For more information visit our product page
for Refractometers [Click Here](#)

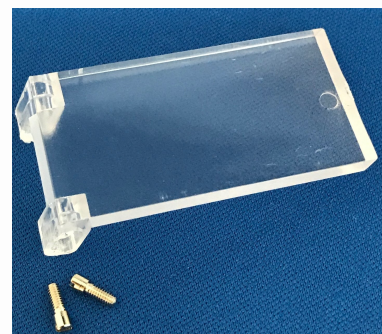

Continued...

Method of operation:

1) Aim the front end of the refractometer to the direction of bright light, and adjust the eyepiece until the reticle can be seen clearly.

2) Adjustment of null:

Open the daylight plate and place 2-3 drops of distilled water on the main prism. Close the daylight plate and press it lightly so the water spreads across the entire surface of the prism without air bubbles or dry spots. Allow the sample to remain on the prism for approximately 30 seconds. **Then adjust** the Calibration Screw until the light/dark boundary coincides with the null line. Adjustment of refractometer with temperature compensation function should be made under the condition of 20°C(68°F) environmental temperature. When working temperature of the room or environment (not the sample) changes by more than 5°F, we recommend recalibration to maintain accuracy.

3) Operation procedure is done after calibration and it is done in essentially the same manner as calibration. Open the daylight plate. Clean the surface of prism by soft cotton cloth. Drop 2-3 drops of solution to be measured on the main prism. Close the daylight plate and press it lightly, then read the corresponding scale of light/dark boundary. The reading is the value of measured solution.

4) After measurement, clean away the measured solution on the surface of prism and cover plate by moist cotton cloth,. After drying, it should be stored perfectly.

Warnings- Maintenance:

1) Adjustment of null: Liquid and specimen should be under the same temperature. If the temperature varies greatly, the null point should be adjusted once per 30 minutes.

2) After usage, don't use water to wash the instrument, so as to prevent water from entering into the instrument.

3) As it is a kind of precision optical instrument, you should handle it gently and take good care of it. Don't touch and scratch the optical surfaces. It should be kept in the environment of dry, clean and non-corrosive air, so as to prevent the surface of it from turning mouldy and foggy. Please avoid strong shock during transportation.

4) If the consumers use the instrument in accordance with the mentioned method of usage, it can be guaranteed that the instrument can't break down. The optical performance can't change.

Warranty and Repair Information:

We warrant that all our refractometers are free from defects in material and workmanship for one year from the date of purchase. If the product is found to be defective by us, we will repair or replace the unit without charge. And we reserve the exclusive right to determine the cause of failure and advise if a warranty replacement or repair can be made. This warranty does not include shipping costs, collect shipments will not be accepted, or any instrument that has become worn through use, broken from mis-use, neglect, tampering, or unauthorized repair. Return shipments will be re-paid freight unless other arrangements have been made. We will advise the customer of the repair cost of any refractometer not covered by warranty. Work on such units will not begin until a purchase order is received. There are no other expressed or implied warranties.

Please call the dealer prior to returning any products for evaluation.

Vetlab Supplies Ltd is a leading supplier of...

- Veterinary Equipment
- Microscopes
- Centrifuges
- Veterinary Diagnostic Test Kits
- Laboratory Consumables

Visit Our Website www.vetlabsupplies.co.uk